

ANALOGUE
A TYPE
P. 00 2
L. 00 1
L. 00 1

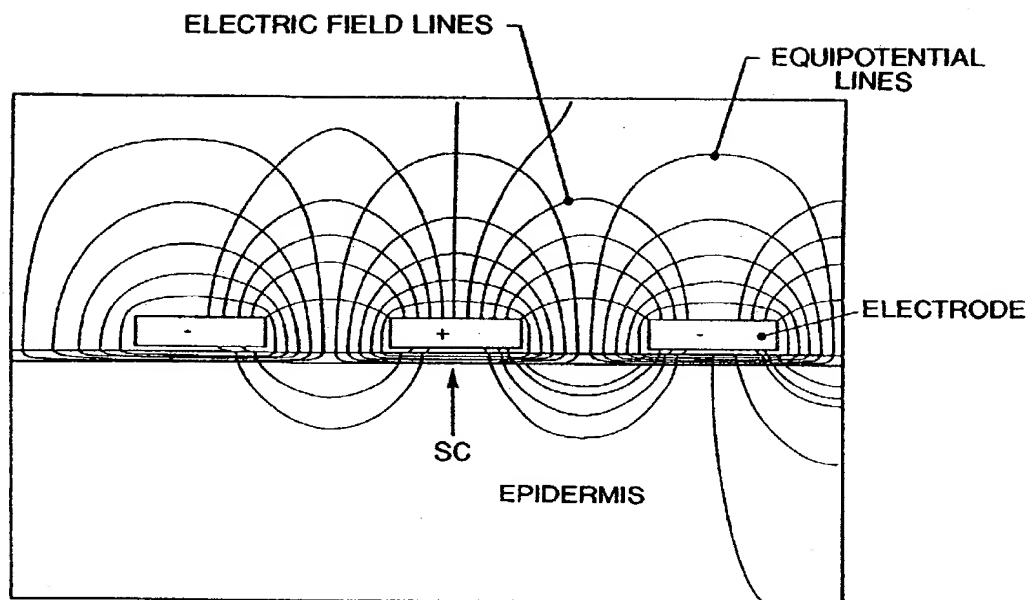


FIG. 2

FIELD STRENGTH BELOW AN ELECTRODE
BEFORE BREAKDOWN OF THE S.C.

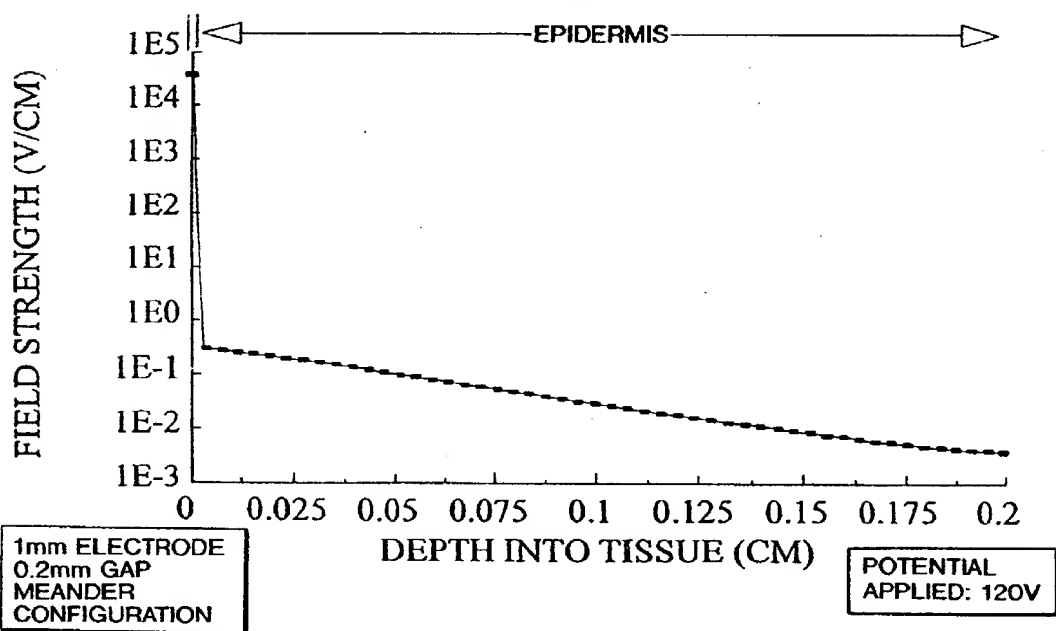


FIG. 3A

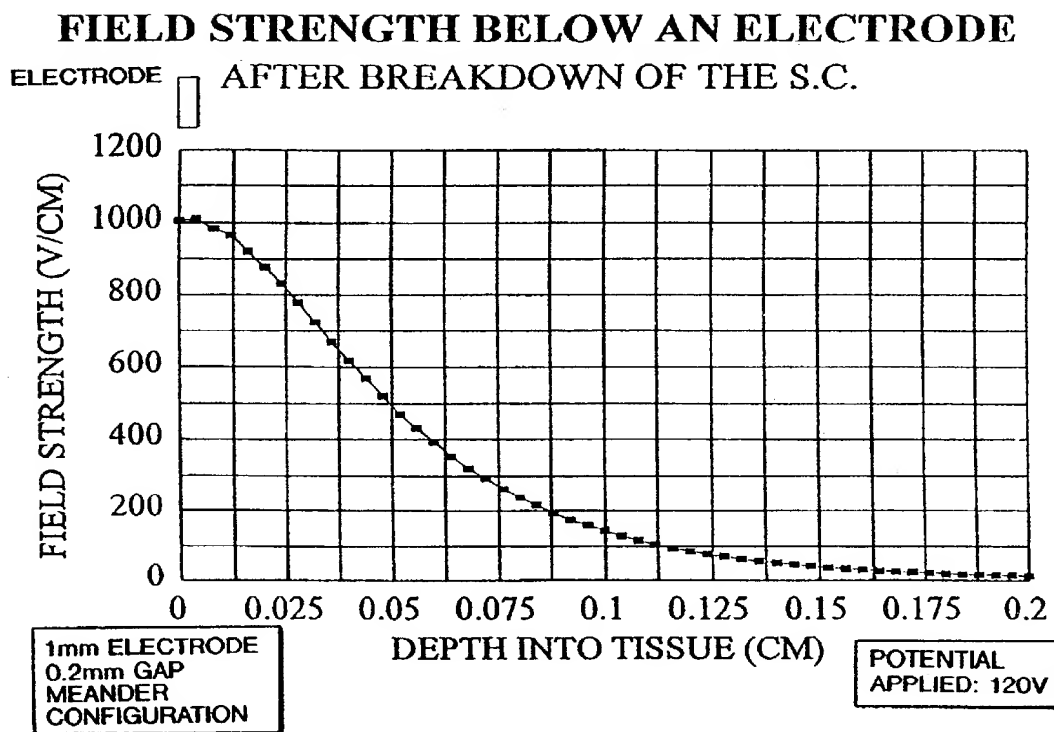


FIG. 3B

50H 72
TAPING
C. A. 1000000
1000000
1000000

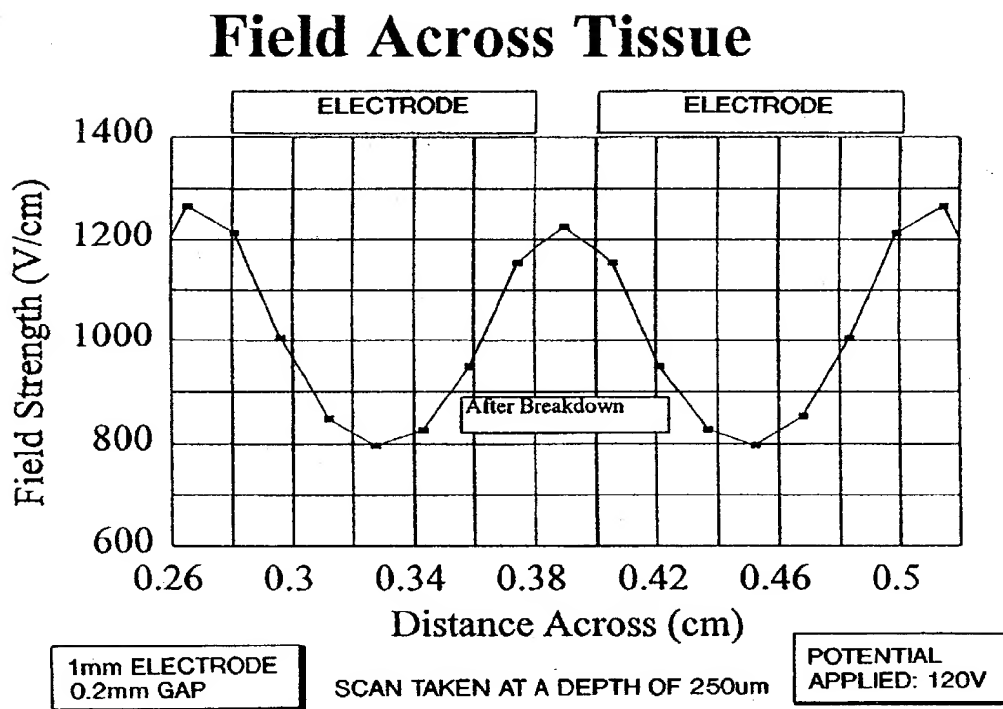


FIG. 4A

Field Across Tissue

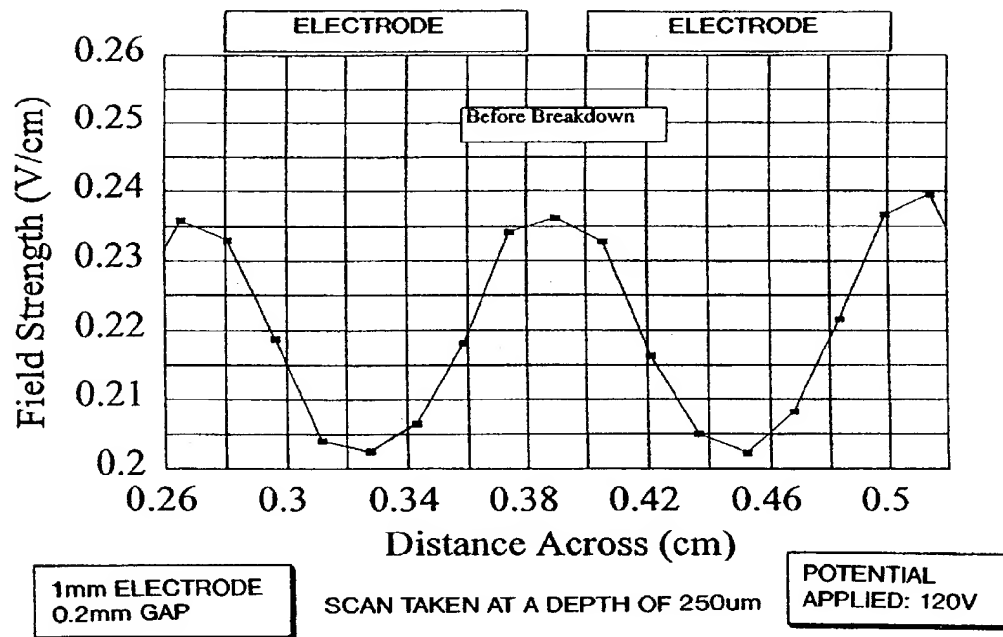


FIG. 4B

BATTERY-POWERED
HAND HELD PULSER

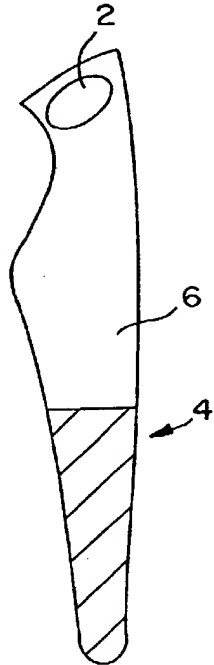


FIG. 5A

BATTERY-POWERED
HAND HELD PULSER

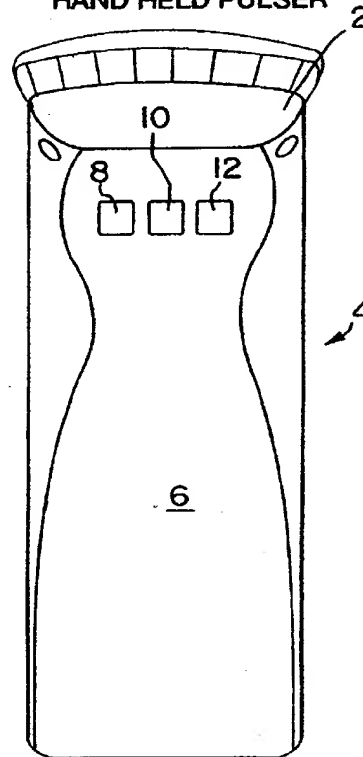


FIG. 5B

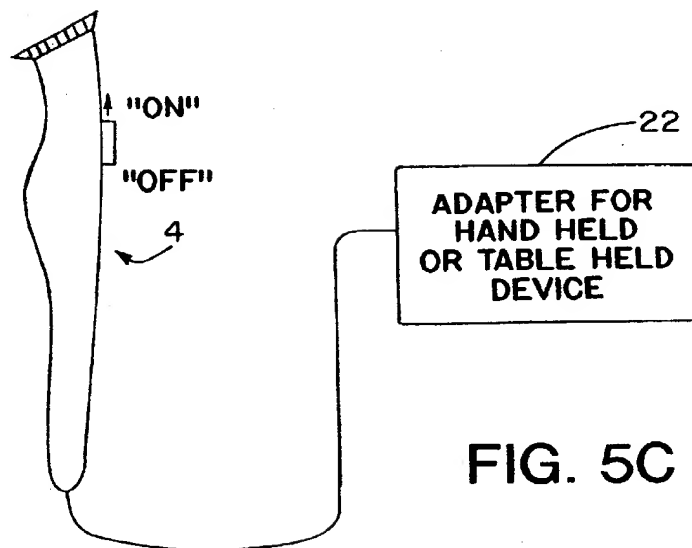


FIG. 5C




FIG. 6A

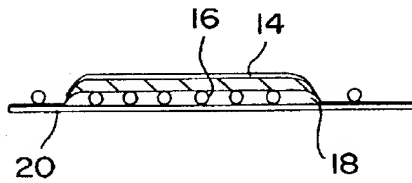


FIG. 6B



FIG. 6C




FIG. 6D




FIG. 6E